

PA 1170654

15.06.2004
REC'D 05 JUL 2004
WIPO PCT

THE UNITED STATES OF AMERICA

TO ALL TO WHOM THESE PRESENTS SHALL COME:

UNITED STATES DEPARTMENT OF COMMERCE

United States Patent and Trademark Office

May 17, 2004


THIS IS TO CERTIFY THAT ANNEXED HERETO IS A TRUE COPY FROM THE RECORDS OF THE UNITED STATES PATENT AND TRADEMARK OFFICE OF THOSE PAPERS OF THE BELOW IDENTIFIED PATENT APPLICATION THAT MET THE REQUIREMENTS TO BE GRANTED A FILING DATE UNDER 35 USC 111.

APPLICATION NUMBER: 60/550,745
FILING DATE: March 05, 2004

PRIORITY DOCUMENT

SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH RULE 17.1(a) OR (b)

By Authority of the
COMMISSIONER OF PATENTS AND TRADEMARKS

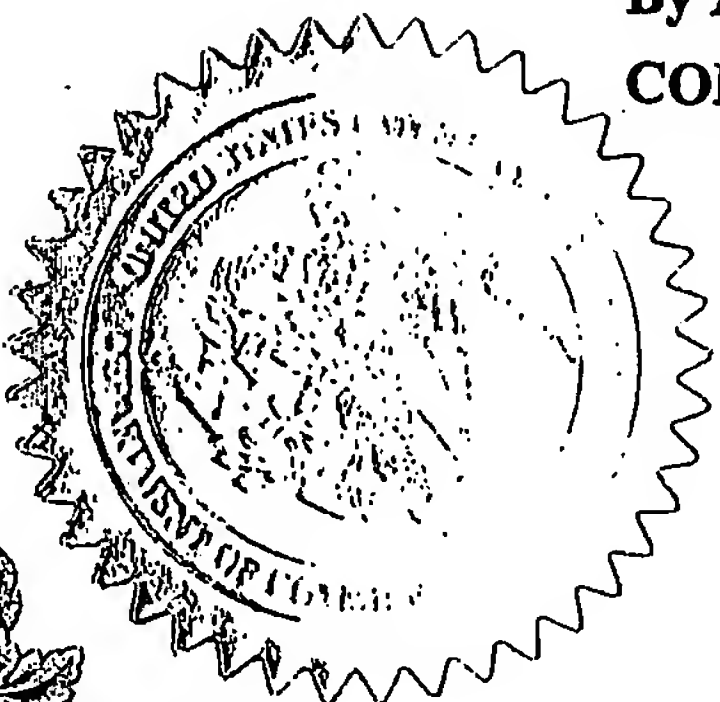

W. Montgomery
W. MONTGOMERY
Certifying Officer

PATENT APPLICATION SERIAL NO. _____

U.S. DEPARTMENT OF COMMERCE
PATENT AND TRADEMARK OFFICE
FEE RECORD SHEET

03/10/2004 CCHAU1 00000052 60550745

01 FC:1005

160.00 DP

PTO-1556
(5/87)

*U.S. Government Printing Office: 2001 — 481-637/59173

030504

21861 U.S. PTO


Please type a plus sign (+) inside this box PTO/SB/16 (5-03)
Approved for use through 04/30/2003. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.**PROVISIONAL APPLICATION FOR PATENT COVER SHEET**

This is a request for filing a PROVISIONAL APPLICATION FOR PATENT under 37 CFR 1.53(c).

INVENTOR(S)					
Given Name (first and middle [if any])		Family Name or Surname		Residence (City and either State or Foreign Country)	
<input type="checkbox"/> Additional inventors are being named on the _____ separately numbered sheets attached hereto					
TITLE OF THE INVENTION (280 characters max)					
CONTACTLESS DETECTION CELL					
Direct all correspondence to: CORRESPONDENCE ADDRESS					
<input checked="" type="checkbox"/> Customer Number		2512		<div>Place Customer Number Bar Code Label here</div>	
OR		Type Customer Number here			
<input type="checkbox"/> Firm or Individual Name					
Address					
Address					
City		State		ZIP	
Country		Telephone		Fax	
ENCLOSED APPLICATION PARTS (check all that apply)					
<input checked="" type="checkbox"/> Specification		Number of Pages		<input type="checkbox"/> CD(s), Number	
<input checked="" type="checkbox"/> Drawing(s)		Number of Sheets		<input type="checkbox"/> Other (specify)	
<input type="checkbox"/> Application Data Sheet. See 37 CFR 1.76					
METHOD OF PAYMENT OF FILING FEES FOR THIS PROVISIONAL APPLICATION FOR PATENT (check one)					
<input checked="" type="checkbox"/> A check or money order is enclosed to cover the filing fees				FILING FEE AMOUNT (\$)	
<input checked="" type="checkbox"/> The Director is hereby authorized to charge filing fees or credit any overpayment to Deposit Account Number:		16-1350		\$160.00	
<input type="checkbox"/> Payment by credit card. Form PTO-2038 is attached.					
The invention was made by an agency of the United States Government or under a contract with an agency of the United States Government.					
<input checked="" type="checkbox"/> No.					
<input type="checkbox"/> Yes, the name of the U.S. Government agency and the Government contract number are: _____					

Respectfully submitted,

SIGNATURE

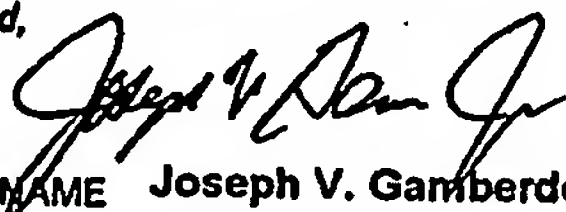

Date

3/5/04

TYPED or PRINTED NAME

Joseph V. Gamberdell, Jr.

REGISTRATION NO.

44,695

(if appropriate)

Docket Number:

860P011716-US(#1)/20031343-1

TELEPHONE


(203) 259-1800

USE ONLY FOR FILING A PROVISIONAL APPLICATION FOR PATENT

This collection of information is required by 37 CFR 1.51. The information is used by the public to file (and by the PTO to process) a provisional application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 8 hours to complete, including gathering, preparing, and submitting the complete provisional application to the PTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Mail Stop Provisional Application, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

P18LARGE/REV05

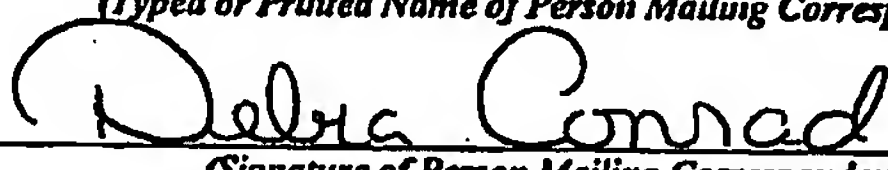CERTIFICATE OF MAILING BY "EXPRESS MAIL" (37 CFR 1.10)			Docket No.
Applicant(s):			860P011716-US(#1)/20031343-1
Serial No. To Be Assigned	Filing Date Herewith	Examiner	Group Art Unit
Invention: CONTACTLESS DETECTION CELL			
<p>I hereby certify that the following correspondence:</p> <div style="border: 1px solid black; padding: 5px; margin: 10px 0;">New United States Provisional Patent Application, Transmittal, 5 Drawings, Check for Payment of Fee & Return Postcard</div> <p style="text-align: center;"><i>(Identify type of correspondence)</i></p> <p>is being deposited with the United States Postal Service "Express Mail Post Office to Addressee" service under 37 CFR 1.10 in an envelope addressed to: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450 on <u>March 5, 2004</u></p> <p style="text-align: center;"><i>(Date)</i></p> <div style="text-align: center; margin-top: 20px;"><u>Debra Conrad</u> <i>(Typed or Printed Name of Person Mailing Correspondence)</i>  <i>(Signature of Person Mailing Correspondence)</i> <u>EV 327693428 US</u> <i>(Express Mail Mailing Label Number)</i></div> <p style="text-align: center; margin-top: 50px;">Note: Each paper must have its own certificate of mailing.</p>			

P08A/REV02

CONTACTLESS DETECTION CELL

BACKGROUND OF THE INVENTION

The present invention relates to a contactless detection cell for detecting an electrical property of one or more sample compounds in a flow path, to a separation
5 system comprising a contactless detection cell, and to a method for increasing the sensitivity of a contactless detection cell.

Contactless detection of an electrical property of sample compounds has become an important alternative to optical detection techniques. For example, in the field of analyzing ions in liquid samples, contactless conductivity detection (CCD) has
10 become a competitive technique. The present invention can be applied to contactless detection of any electrical property.

SUMMARY OF THE INVENTION

It is an object of the invention to provide an improved contactless detection of an electrical property of one or more sample compounds in a flow path. The object is
15 solved by the independent claims. Preferred embodiments are shown by the dependent claims.

According to embodiments of the present invention, a contactless detection cell for detecting an electrical property of one or more sample compounds in a flow path is provided. The contactless detection cell comprises a transmitter electrode adapted
20 for capacitively coupling an AC current into a detection channel of the flow path, and a receiver electrode adapted for receiving the AC current that has been coupled into the detection channel. An inner cross-section in at least a section of the detection channel is different than an inner cross-section of the flow path towards the detection channel.

25 When the inner cross-section in at least a section of the detection flow path is varied

independently of the dimensions of the preceding flow path, it is possible to optimize the geometry of the detection channel according to the needs imposed by the respective contactless detection technique.

5 There exist a variety of different parameters that describe the behaviour of a contactless detection cell. According to embodiments of the present invention, one or more of said parameters can be affected by adjusting the geometry of the detection channel. One important parameter is the separation power of the contactless detection cell, which determines the resolution of the obtained results. A further aspect is cross-talk between the transmitter electrode and the receiver
10 electrode, which impairs the quality of the obtained results or spectra. Cross talk occurs if the AC field emitted by the transmitter electrode is directly received by the receiver electrode, without passing through the sample volume.

Another important parameter is the detection cell's sensitivity. A detection cell with high sensitivity allows detecting small concentrations of sample compounds. The
15 more sensitive the cell is, the smaller the respective limits of detection (LODs) for the various compounds will be. Sensitivity is closely related to the signal-to-noise ratio of the measurement, whereby a large signal-to-noise ratio corresponds to a high sensitivity.

By choosing the inner cross-section of at least a part of the detection channel
20 independently of the preceding flow path's cross section, an additional degree of freedom is gained. This additional degree of freedom can e.g. be used for improving any property of the detection cell, for example for at least one of: increasing the separation power, improving the signal-to-noise ratio, reducing cross talk, etc. Besides that, this additional degree of freedom might as well be used for modifying
25 any other property of the detection cell that has not been mentioned yet, in order to improve the detection cell's properties in a given context.

According to a preferred embodiment of the invention, the resistance of the sample

volume in the detection channel is increased by lowering the inner cross section of the detection flow path between the transmitter electrode and the receiver electrode. By narrowing the detection channel, the sample volume is stretched and spread out, and its resistance is increased. As a consequence, variations in resistance caused
5 by the various sample compounds are enhanced and can be monitored more precisely. The signal-to-noise level is increased, and the detection cell's sensitivity is improved. Furthermore, by narrowing the detection channel, the analyte's resistance becomes the most significant contribution to the overall impedance measured between the electrodes.

10 In another embodiment of the invention, the transmitter electrode and the receiver electrode are arranged in an axial geometry. In case the detection cell volume is kept sufficiently small, the axial approach allows to record the analyte bands with good resolution.

According to a preferred embodiment, the transmitter electrode and the receiver
15 electrode are separated by a distance that is sufficiently large for reducing or even avoiding distortions related to cross-talk. On the one hand, by increasing the distance between the electrodes, the amount of cross-talk can be reduced. On the other hand, by increasing the distance between the electrodes, the detection cell's volume might be increased as well, and as a consequence, the resolution of the
20 obtained measurements might be lowered. However, by reducing the inner cross section, the detection cell volume can be kept small without bringing the electrodes too close together. Hence, it is possible to provide a detection cell with a small detection cell volume and with electrodes that are axially spaced apart by a rather large distance. As a result, the detection cell has low susceptibility to cross talk and
25 yields high-resolution measurements.

According to a preferred embodiment of the invention, the inner cross-section of the detection channel is kept small throughout the detection channel. Within the entire detection channel, the inner cross-section is constant. This might e.g. be

advantageous from a manufacturing point of view.

According to an alternative embodiment, the inner cross-section of the detection channel is axially varied in a way that, at the locations of the electrodes, its inner diameter is large, whereas between the electrodes, its inner cross-section is small.

5 Thus, an hour-glass shaped detection channel is obtained. This geometry might also be referred to as an "inverted bubble". By increasing the inner diameter at the sites where the ring-shaped electrodes are located, the capacitive coupling between the transmitter electrode and the sample is improved, and the capacitive coupling between the receiver electrode and the sample is improved as well. Together with
10 the sample, the respective electrode represents a capacitance. By increasing the inner diameter of the detection channel at the locations of the electrodes, the effective "surface" of the respective capacitance is increased, while the distance between the sample and the electrode is decreased. As a result, the respective capacitances are increased. Due to the improved capacitive coupling, the resistance
15 of the sample between the electrodes can be measured more accurately, because it provides the major contribution to the total (complex) impedance between the electrodes.

In a preferred embodiment, the detection channel is implemented by means of a capillary with a reduced inner cross-section in the portion between the transmitter
20 electrode and the receiver electrode. One common way of realizing a migration flow path is to use a glass capillary.

In a preferred embodiment, between the transmitter electrode and the receiver electrode, the inner diameter of the capillary is equal to about 0.1 μm to 200 μm , further preferably 1.0 μm to 20 μm . Between the electrodes, the ratio of the
25 capillary's outer diameter to the capillary's inner diameter is equal to about 1.1 to 50, preferably 1.5 to 10.

According to an alternative embodiment of the invention, the detection channel

shape is implemented using microstructuring technologies as common for making microfluidic chip devices. Such microstructuring technologies might e.g. include etching, laser ablation, direct molding. Using these techniques, the detection channel can be shaped with high precision. Microsystem technologies allow for an accurate
5 positioning of contactless electrodes relative to the detection volume. In yet another preferred embodiment, the detection channel is implemented as a part of a microfluidic chip device.

In a further preferred embodiment, the electrical property is at least one of: conductivity, complex conductivity, impedance, resistance, reactance, relative
10 permittivity. When an analyte band passes through the detection cell, any of these electrical properties might be modified. Hence, by monitoring the respective electrical property, it is possible to detect the respective analyte band. In particular, the detection cell might e.g. be adapted for detecting conductivity of the sample compounds. In this case, the detection cell is commonly referred to as a contactless
15 conductivity detection (CCD) cell. The present invention is not limited to CCD detection, though.

According to a preferred embodiment, the one or more sample compounds have been separated in a preceding separation flow path. First, the various sample compounds are separated as they migrate through the separation flow path. Then,
20 the analyte bands can be analyzed by the detection cell.

According to another preferred embodiment, the inner cross-section of the detection channel is smaller than the inner cross-section of the flow path towards the detection channel. In the separation flow path, it might be advantageous to use a large-bore capillary, because a large-bore capillary provides a sufficient sample loading
25 capability. A large-bore capillary allows to inject a well-defined sample plug of sufficient volume into the separation flow path. However, in the detection flow path, it might be advantageous, especially with regard to cross talk, sensitivity, separation power, etc., to utilize a capillary with a rather small inner diameter.

According to an alternative embodiment, the inner cross-section of the detection channel might as well be greater than the inner cross-section of the flow path towards the detection channel.

5 A separation system according to embodiments of the present invention comprises a separation flow path adapted for separating sample compounds of a given sample, and a contactless detection cell of the type described above.

10 According to a preferred embodiment, the separation system is at least one of: an electrophoresis system, a liquid chromatography system, an electrochromatography system, or a combination thereof. The contactless detection cell can be used together with each of these techniques.

15 In a preferred embodiment, the separation system is employed for ion analysis. The presence of ions or ionizable compounds in the sample modifies the conductivity of the sample, and for this reason, contactless detection, in particular CCD, is well-suited for detecting analyte bands that correspond to different types of ions or ionizable compounds. Ion analysis might e.g. be employed for analysing beverages (beer, wine, mineral water, juice, etc.), for analysing cooling water of a power plant, etc.

20 Furthermore, embodiments of the present invention relate to a method for increasing the sensitivity of a contactless detection cell, with said detection cell being adapted for detecting an electrical property of one or more sample compounds. The detection cell comprises a transmitter electrode adapted for capacitively coupling an AC signal into a detection channel and a receiver electrode adapted for receiving an AC response signal in response to the AC signal that has been coupled into the detection channel. The method comprises a step of reducing, in at least a section of
25 the detection channel, the inner cross-section of the detection channel relative to the inner cross-section of the flow path towards the detection channel.

BRIEF DESCRIPTION OF THE DRAWINGS

Other objects and many of the attendant advantages of the present invention will be readily appreciated and become better understood by reference to the following detailed description when considering in connection with the accompanied drawings. Features that are substantially or functionally equal or similar will be referred to with
5 the same reference sign(s).

- Fig. 1 shows a measurement set-up comprising a contactless detection cell;
- Fig. 2 shows a detection flow path according to a first embodiment of the invention;
- Fig. 3 depicts three electropherograms that have been recorded for three
10 different inner diameters of the detection channel;
- Fig. 4 shows a detection flow path according to another embodiment of the invention; and
- Fig. 5 shows an equivalent circuit of a contactless detection cell.

15 DETAILED DESCRIPTION OF EMBODIMENTS OF THE INVENTION

In Fig. 1, a measurement set-up comprising a contactless detection cell is depicted. The contactless detection cell 1 is adapted for detecting compounds that have migrated through a preceding separation flow path 2, whereby the separation flow path 2 might e.g. be part of a capillary electrophoresis (CE) system, or of a liquid
20 chromatography (LC) system, etc. The contactless detection cell 1 comprises a transmitter electrode 3 that is adapted for applying an AC field to the detection volume 4, and a receiver electrode 5 that is adapted for detecting the AC current that passes through the detection volume 4. The transmitter electrode 3 and the receiver electrode 5 are arranged in an axial geometry, which means that they are spaced
25 apart by a certain distance in the direction of the flow. The transmitter electrode 3 is

connected to a high frequency (HF) AC power supply 6 that provides a HF AC voltage signal 7 to the transmitter electrode 3, whereby the frequency of the HF AC voltage might e.g. range from several kHz to several hundred MHz. The amplitude of the HF AC voltage signal is determined by a control voltage 8 that is input to the
5 HF AC power supply 6.

The receiver electrode 5 is connected to a current/voltage converter 9, which is adapted for converting the received AC current into a corresponding voltage signal. This voltage signal is provided to a rectifier and filter unit 10. At the output of the rectifier and filter unit 10, an analogue DC signal 11 is obtained, with said DC signal
10 11 indicating the conductivity of the detection volume 4. By means of an analogue/digital converter 12, the analogue DC signal 11 is converted into a corresponding conductivity read-out 13.

Fig. 2 shows the geometry of a contactless detection cell according to an embodiment of the present invention. In Fig. 2, a part of the separation flow path 14
15 is shown together with a contactless detection cell 15. The contactless detection cell 15 comprises a transmitter electrode 16 that is implemented as a ring-shaped electrode. The ring-shaped electrode and the solute form a capacitance, and via said ring-shaped electrode, an AC current can be capacitively coupled to the solute. The receiver electrode 17 is axially separated from the transmitter electrode 16 by an
20 axial distance L. The receiver electrode 17 is also realized as a ring-shaped electrode, with said ring-shaped electrode and the solute forming a capacitance. The receiver electrode 17, which is capacitively coupled to the solute, may receive and detect an AC current that has been coupled to the solvent via the transmitter electrode 16.

25 By recording electrical properties of the solvent as a function of time, it is possible to detect the various different analyte bands. The separation power of the contactless detection cell 15 is mainly determined by the detection volume encompassed between the transmitter electrode 16 and the receiver electrode 17. Of course, one

might think of bringing the two electrodes rather close together, in order to improve the resolution. However, if the electrodes are brought within close proximity of each other, a phenomenon referred to as cross talk will deteriorate the obtained signal. Cross talk occurs if the AC field emitted by the transmitter electrode is directly
5 received by the receiver electrode, without passing through the sample volume.

The following example calculation will help to understand how the half-width of an analyte band that migrates through the separation flow path can be determined. The axial dispersion due to diffusion, s^2 , is given by the formula

$$s^2 = 2 D \cdot t$$

10 with D being the diffusion coefficient, and with t being the migration time. Typical diffusion coefficients of medium-molecular analytes range from $2 \times 10^{-10} \text{ m}^2 \text{ s}^{-1}$ to $5 \times 10^{-10} \text{ m}^2 \text{ s}^{-1}$, and typical migration times range from 30s to 100s. When the lower limits of these ranges are inserted into the above equation, the axial dispersion of the analyte band is obtained as $s^2 = 1.2 \times 10^{-8} \text{ m}^2$. In case a Gaussian shape of the
15 analyte band is assumed, the half-width p of the analyte band can be expressed as $p = 2.35 s \approx 0.25 \text{ mm}$.

This result shows that for detecting the analyte bands with good resolution, the two electrodes of the detection cell have to be moved very close together. However, if the electrodes are moved that close together, cross talk will occur, which means that the
20 HF field emitted by the transmitter electrode will be directly coupled to the receiver electrode, and the detected AC signal will be disturbed.

According to embodiments of the present invention, at least in a part of the flow path between the two electrodes, the inner diameter of the detection flow path is reduced. As a consequence, the detection cell volume is decreased without bringing the
25 electrodes too close together.

In the embodiment shown in Fig. 2, the inner diameter ID_{DET} of the detection flow path

is considerably smaller than the inner diameter ID_{SEP} of the preceding separation flow path. Between the two portions of the flow path, a shoulder 18 is formed. The rather small volume of the detection cell allows to separately detect each of the analyte bands with sufficient resolution. By reducing the detection cell volume, the separation
5 power of the instrument is improved. The transmitter electrode 16 and the receiver electrode 17 can be placed sufficiently far apart from each other to avoid – or at least reduce – cross talk between them, whereby the detection cell volume still remains sufficiently small for obtaining a good resolution.

There is still another reason why the distance L between the transmitter electrode 16
10 and the receiver electrode 17 should not become too small. The AC current that passes through the detection cell tends to heat up the detection cell. Therefore, cooling facilities have to be provided, in particular at the portion of the detection flow path between the transmitter electrode 16 and the receiver electrode 17. In this respect, it is advantageous if the distance L between the two electrodes does not
15 become too small.

As the inner diameter ID_{SET} of the separation flow path 14 is rather large and exceeds the inner diameter ID_{DET} of the detection flow path, it is possible to inject a sample plug of considerable volume into the separation flow path, whereby said sample plug does not spread too much in the axial direction. With $ID_{SEP} > ID_{DET}$, a superior
20 definition of the injection plug is obtained. The sample-loading capability of the large-bore capillary of the separation flow path can be combined with the superior separation power and sensitivity of the narrow-bore capillary that is employed in the detection flow path.

The separation flow path and the detection flow path can be implemented by means
25 of a glass capillary having two different inner cross sections. The inner diameter ID_{DET} in the portion of the detection cell might e.g. be equal to 50 μm , while the glass capillary's outer diameter OD might be as large as 360 μm , in order to avoid disruptive discharge (or HV breakdown).

Instead of utilizing a glass capillary, the electromigration channel and the detection flow path might as well be realized by means of a microfluidic chip device. The microfluidic chip device allows for more convenient ways of shaping the geometry of the flow path. Microfluidic chips commonly comprise two or more substrates that are arranged in a sandwich layer structure. The structure can e.g. be crafted by etching, laser ablation or by direct molding. Then, the different substrates are annealed or bonded. Microsystem technologies allow for a precise positioning of the electrodes relative to the detection channel.

Another important property in the field of contactless detection is the signal-to-noise ratio of the recorded signal. The signal-to-noise ratio is a measure for the system's sensitivity, whereby a large signal-to-noise ratio corresponds to a high sensitivity. In Fig. 3, three different electrophoresis contactless conductivity detector traces are shown. In the following, the measuring conditions are given in more detail:

15	Buffer:	Agilent Basic Anion Buffer (PN 5064-8209)
	Sample:	Phosphate 100 mg/l, Carbohydrates 200 mg/l each, others 50 mg/l each
	Preconditioning:	4 min at run buffer
	Capillary:	fused silica
20	Injection:	400 mbar*s
	Temperature:	30°C
	Voltage:	-20 kV (reversed polarity)
	Current:	-36 μ A
25	Detection:	CCD Data Rate 2 Hz

The respective CCD signals are depicted as a function of time, whereby curve 19 corresponds to an inner diameter of 75 μ m, whereby curve 20 relates to ID = 50 μ m, and whereby curve 21 has been recorded utilizing a capillary with an inner diameter of 20 μ m. In order to simplify the comparison of the respective signal-to-noise ratios of curves 19, 20, 21, the curves have been individually scaled in a way that their respective noise levels have been brought to one common value. An offset is added

to bring these traces inside a common window.

The electropherogram that has been recorded for a narrow-bore capillary (ID = 20 μm) shows the largest peaks, whereas the electropherogram obtained for the large-bore capillary (ID = 75 μm) comprises peaks of a relatively small height. By utilizing
5 a detection flow path with a small inner diameter (ID = 20 μm), an excellent signal-to-noise ratio can be achieved, whereas a capillary with a large inner diameter (ID = 75 μm) leads to a signal-to-noise ratio that is considerably smaller. The conclusion is that by reducing the inner diameter within the detection flow path, or within parts thereof, it is possible to improve both the separation power (resolution) and the
10 sensitivity (the signal-to-noise ratio) of the contactless detection. Though the absolute amount of the respective sample compound encompassed between the two electrodes becomes smaller when the inner diameter is reduced, a superior signal quality is obtained.

The increase in sensitivity can also be expressed in terms of the limit of detection
15 (LOD), which is defined as the minimum concentration of a certain substance that allows to distinguish the corresponding measurement peak from the underlying noise level. By reducing the inner diameter of the detection flow path, the limit of detection for the respective sample compound is decreased.

Fig. 4 shows another embodiment of the present invention. Sample compounds that
20 have migrated through a separation flow path 22 are subsequently analyzed by a contactless detection cell 23. Between the electrodes 24, 25, the inner diameter ID_{DET} of the detection channel is reduced relative to the inner diameter ID_{SEP} of the preceding separation flow path 22. Thus, the volume of the detection cell volume 26 is decreased without reducing the distance between the two electrodes 24, 25. By
25 decreasing the detection cell volume 26, both resolution and sensitivity of the contactless detection cell can be improved. Furthermore, at the sites 27, 28 of the flow path where the electrodes 24, 25 are located, the respective inner diameters ID_{C1} and ID_{C2} are increased relative to the inner diameter ID_{DET} in the section of the

flow path between the electrodes 24, 25, and an hour-glass shaped geometry of the detection cell is obtained. In this respect, the embodiment shown in Fig. 4 differs from the embodiment of Fig. 2.

Because of $ID_{C1} > ID_{DET}$, the capacitance C_1 formed by the ring-shaped electrode 24 and the sample is increased, and as a consequence, the capacitive coupling between the electrode 24 and the sample is improved. Accordingly, because of $ID_{C2} > ID_{DET}$, the capacitance C_2 formed by the ring-shaped electrode 25 and the sample is increased as well. The arrangement shown in Fig. 4 can be seen as a first complex conductivity $X_{C1} = \frac{1}{i \cdot \omega \cdot C_1}$ that is connected in series with a resistance R of the sample volume between the electrodes, and with a second complex conductivity $X_{C2} = \frac{1}{i \cdot \omega \cdot C_2}$, whereby ω denotes the frequency of the AC signal. By increasing C_1 , C_2 , the contribution of the resistance R is enhanced relative to X_{C1} , X_{C2} . This allows to track changes dR of the resistance R , which might be due to analyte bands that pass through the detection cell, with an improved accuracy.

In Fig. 4, the inner diameter ID_{SEP} is equal to ID_{C1} and ID_{C2} . It has to be pointed out that the inner diameter ID_{SEP} of the separation flow path can be chosen independently of the inner diameters ID_{C1} and ID_{C2} . The inner diameter ID_{SEP} of the separation flow path might as well differ from ID_{C1} and ID_{C2} .

Fig. 5 shows an approximate equivalent circuit of a contactless detection cell. In principle the capacitive coupling of both electrodes, the transmitter electrode and the receiver electrode, to the real electrolyte resistance in the detection channel forms a spatially distributed RC network. Such spatially distributed structures are difficult to analyze precisely, therefore we assume that resistivity of the sample in the detection channel can be equidistantly divided into a number of segments forming individual resistors, $R1-R6$. All the resistors are connected in series. The coupling of the transmitter electrode and the receiver electrode with the solution in the

detection channel is modeled by means of a set of capacitors, C1-C8. Rg is the resistor, which represents the resistivity of the sample placed between the transmitter electrode and the receiver electrode. A possible capacitive crosstalk between both electrodes is modeled by the capacity Cv. Further, U is the voltage of a high
5 frequency AC power supply. The receiver 29 reads the electric current sensed by the receiver electrode.

Such equivalent circuit (possibly using division of the separation channel into more segments) allows with sufficient precision a complete calculation of all complex currents in all loops, as well as the current sensed by the receiver. This enables
10 optimization of the geometry and other parameters of the contactless detection cell.

CLAIMS:

1. A contactless detection cell (15, 23) for detecting an electrical property of one or more sample compounds in a flow path, said contactless detection cell (15, 23) comprising:
 - 5 a transmitter electrode (16, 24) adapted for capacitively coupling an AC current into a detection channel of the flow path;
 - a receiver electrode (17, 25) adapted for receiving the AC current that has been coupled into the detection channel;
 - 10 wherein an inner cross-section in at least a section of the detection channel is different than an inner cross-section of the flow path towards the detection channel.
2. The detection cell of claim 1, wherein the inner cross-section of the detection channel is narrowed between the electrodes in a way that the resistance of the sample volume between the transmitter electrode and the receiver electrode is
15 increased.
3. The detection cell of claim 1 or any one of the above claims, wherein the transmitter electrode and the receiver electrode are axially separated from each other in the flow path.
4. The detection cell of claim 1 or any one of the above claims, wherein the axial
20 separation between the electrodes is sufficiently large for avoiding or at least reducing cross-coupling between the transmitter electrode and the receiver electrode.
5. The detection cell of claim 1 or any one of the above claims, wherein within the
25 entire detection channel, the inner cross section of the detection channel is kept small.

6. The detection cell of claim 1 or any one of the above claims, wherein, at the respective sites (27, 28) of the detection channel where the transmitter electrode (24) and the receiver electrode (25) are located, the detection channel's inner cross-section is larger than the detection channel's inner cross-section in the portion between the electrodes.
7. The detection cell of claim 1 or any one of the above claims, wherein the geometry of the detection channel is axially varied in a way that an hour-glass shaped geometry of the detection channel is obtained.
8. The detection cell of claim 1 or any one of the above claims, wherein the detection channel is implemented by means of a capillary with a reduced inner cross-section in the portion between the transmitter electrode and the receiver electrode.
9. The detection cell of claim 7 or any one of the above claims, wherein in the portion of the detection channel between the electrodes, the inner diameter of the capillary is equal to about 0.1 μm to 200 μm , preferably 1.0 μm to 20 μm .
10. The detection cell of claim 7 or any one of the above claims, wherein in the portion of the detection channel between the electrodes, the ratio of the capillary's outer diameter to the capillary's inner diameter is equal to about 1.1 to 50, preferably 1.5 to 10.
11. The detection cell of claim 1 or any one of the above claims, wherein the detection channel shape is implemented using microstructuring technologies as common for making microfluidic chip devices.
12. The detection cell of claim 1 or any one of the above claims, wherein the detection channel is implemented as a part of a microfluidic chip device.
13. The detection cell of claim 1 or any one of the above claims, wherein the

electrical property is at least one of: conductivity, complex conductivity, impedance, resistance, reactance, relative permittivity.

14. The detection cell of claim 1 or any one of the above claims, wherein the detection cell is adapted for detecting conductivity of the sample compounds.
- 5 15. The detection cell of claim 1 or any one of the above claims, wherein the one or more sample compounds have been separated in a preceding separation flow path.
16. The detection cell of claim 1 or any one of the above claims, wherein the inner cross-section of the detection channel is smaller than the inner cross-section of the flow path towards the detection channel.
- 10 17. The detection cell of claim 1 or any one of the above claims, wherein the inner cross-section of the detection channel is greater than the inner cross-section of the flow path towards the detection channel.
18. A contactless conductivity detection cell for detecting conductivity of sample compounds that have been separated in a preceding separation flow path, said contactless conductivity detection cell comprising
- 15 a transmitter electrode adapted for capacitively coupling an AC current into a detection channel;
- a receiver electrode adapted for receiving the AC current that has been coupled into the detection channel, with the transmitter electrode and the receiver electrode being axially separated;
- 20 a detection channel, wherein the inner cross-section of the detection channel between the transmitter electrode and the receiver electrode is smaller than the inner cross-section of the separation flow path.

19. A separation system comprising
- a separation flow path (14, 22) adapted for separating sample compounds of a given sample;
- a contactless detection cell (15, 23) according to any of claims 1 to 17.
- 5 20. The separation system of claim 19, wherein the separation system is at least one of: an electrophoresis system, a liquid chromatography system, an electrochromatography system, or a combination thereof.
21. The separation system of claim 19 or any one of the above claims, wherein the separation system is adapted for separating and/or analyzing ions.
- 10 22. A method for increasing the sensitivity of a contactless detection cell (15, 23), said detection cell comprising a transmitter electrode (16, 24) adapted for capacitively coupling an AC signal into a detection channel and a receiver electrode (17, 25) adapted for receiving an AC response signal in response to the AC signal that has been coupled into the detection channel, and with said
- 15 detection cell being adapted for detecting an electrical property of one or more sample compounds, the method comprising a step of:
- reducing, in at least a section of the detection channel, the inner cross-section of the detection channel relative to the inner cross-section of the flow path towards the detection channel.
- 20 23. The method of claim 22, wherein the electrical property is at least one of: conductivity, complex conductivity, impedance, resistance, reactance, relative permittivity.
24. The method of claim 22 or any one of the above claims, wherein the detection cell is adapted for detecting conductivity of the sample compounds.

25. The method of claim 22 or any one of the above claims, wherein the one or more sample compounds have been separated in a preceding separation flow path (14, 22).
- 5 26. The method of claim 22 or any one of the above claims, wherein the transmitter electrode and the receiver electrode are axially separated from each other in the flow path.
- 10 27. The method of claim 22 or any one of the above claims, wherein the resistance of the sample volume between the transmitter electrode and the receiver electrode is increased by narrowing the inner diameter of the detection channel between the electrodes.
28. The method of claim 22 or any one of the above claims, wherein the detection channel's volume is reduced while keeping the distance between the electrodes sufficiently large for avoiding or at least reducing cross-coupling between the transmitter electrode and the receiver electrode.
- 15 29. The method of claim 22 or any one of the above claims, comprising a step of increasing the capacitive coupling between the electrodes and the detection channel by increasing the detection channel's inner diameter at the sites of the detection channel where the transmission electrode and the receiver electrode are respectively located.

20

ABSTRACT

A contactless detection cell for detecting an electrical property of one or more sample compounds in a flow path is described. The contactless detection cell comprises a transmitter electrode adapted for capacitively coupling an AC current into a detection
5 channel of the flow path, and a receiver electrode adapted for receiving the AC current that has been coupled into the detection channel. An inner cross-section in at least a section of the detection channel is different than an inner cross-section of the flow path towards the detection channel.

10 (Fig. 4 for publication)

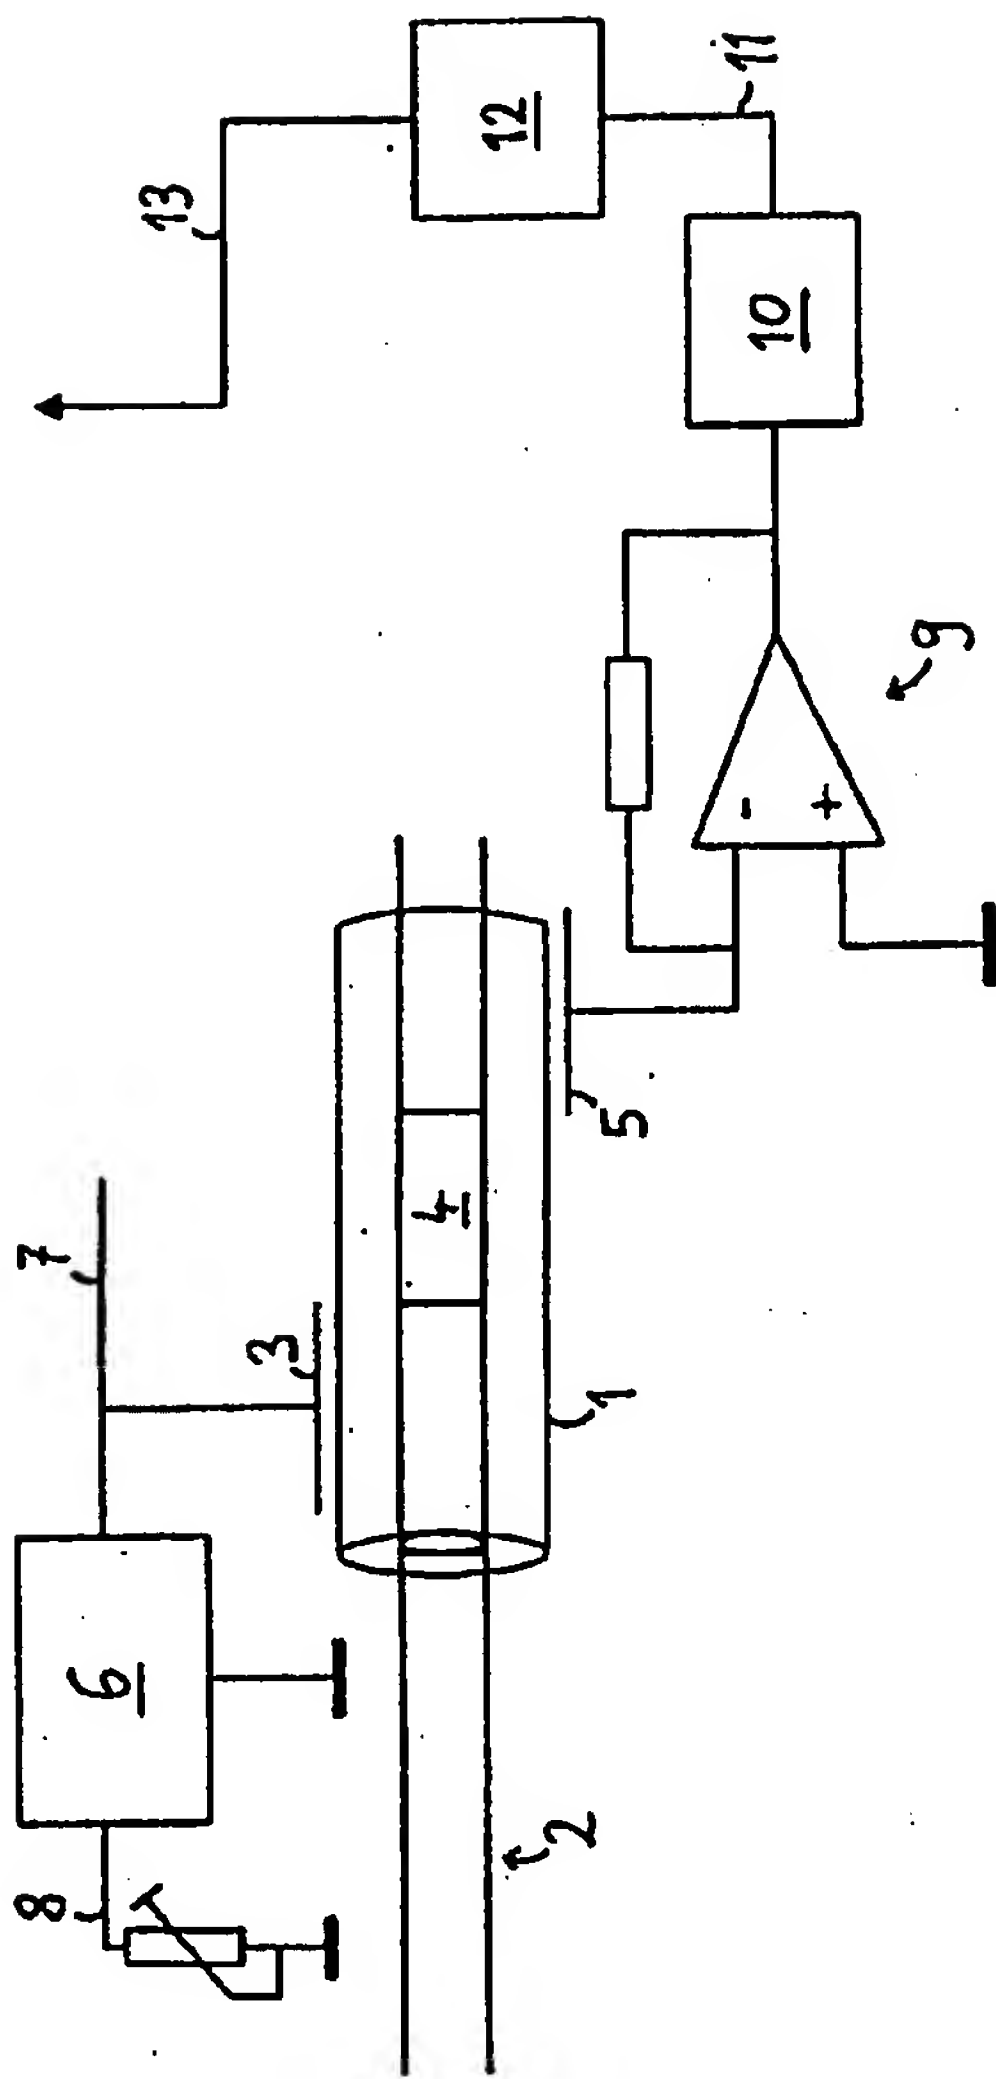


Fig. 1

BEST AVAILABLE COPY

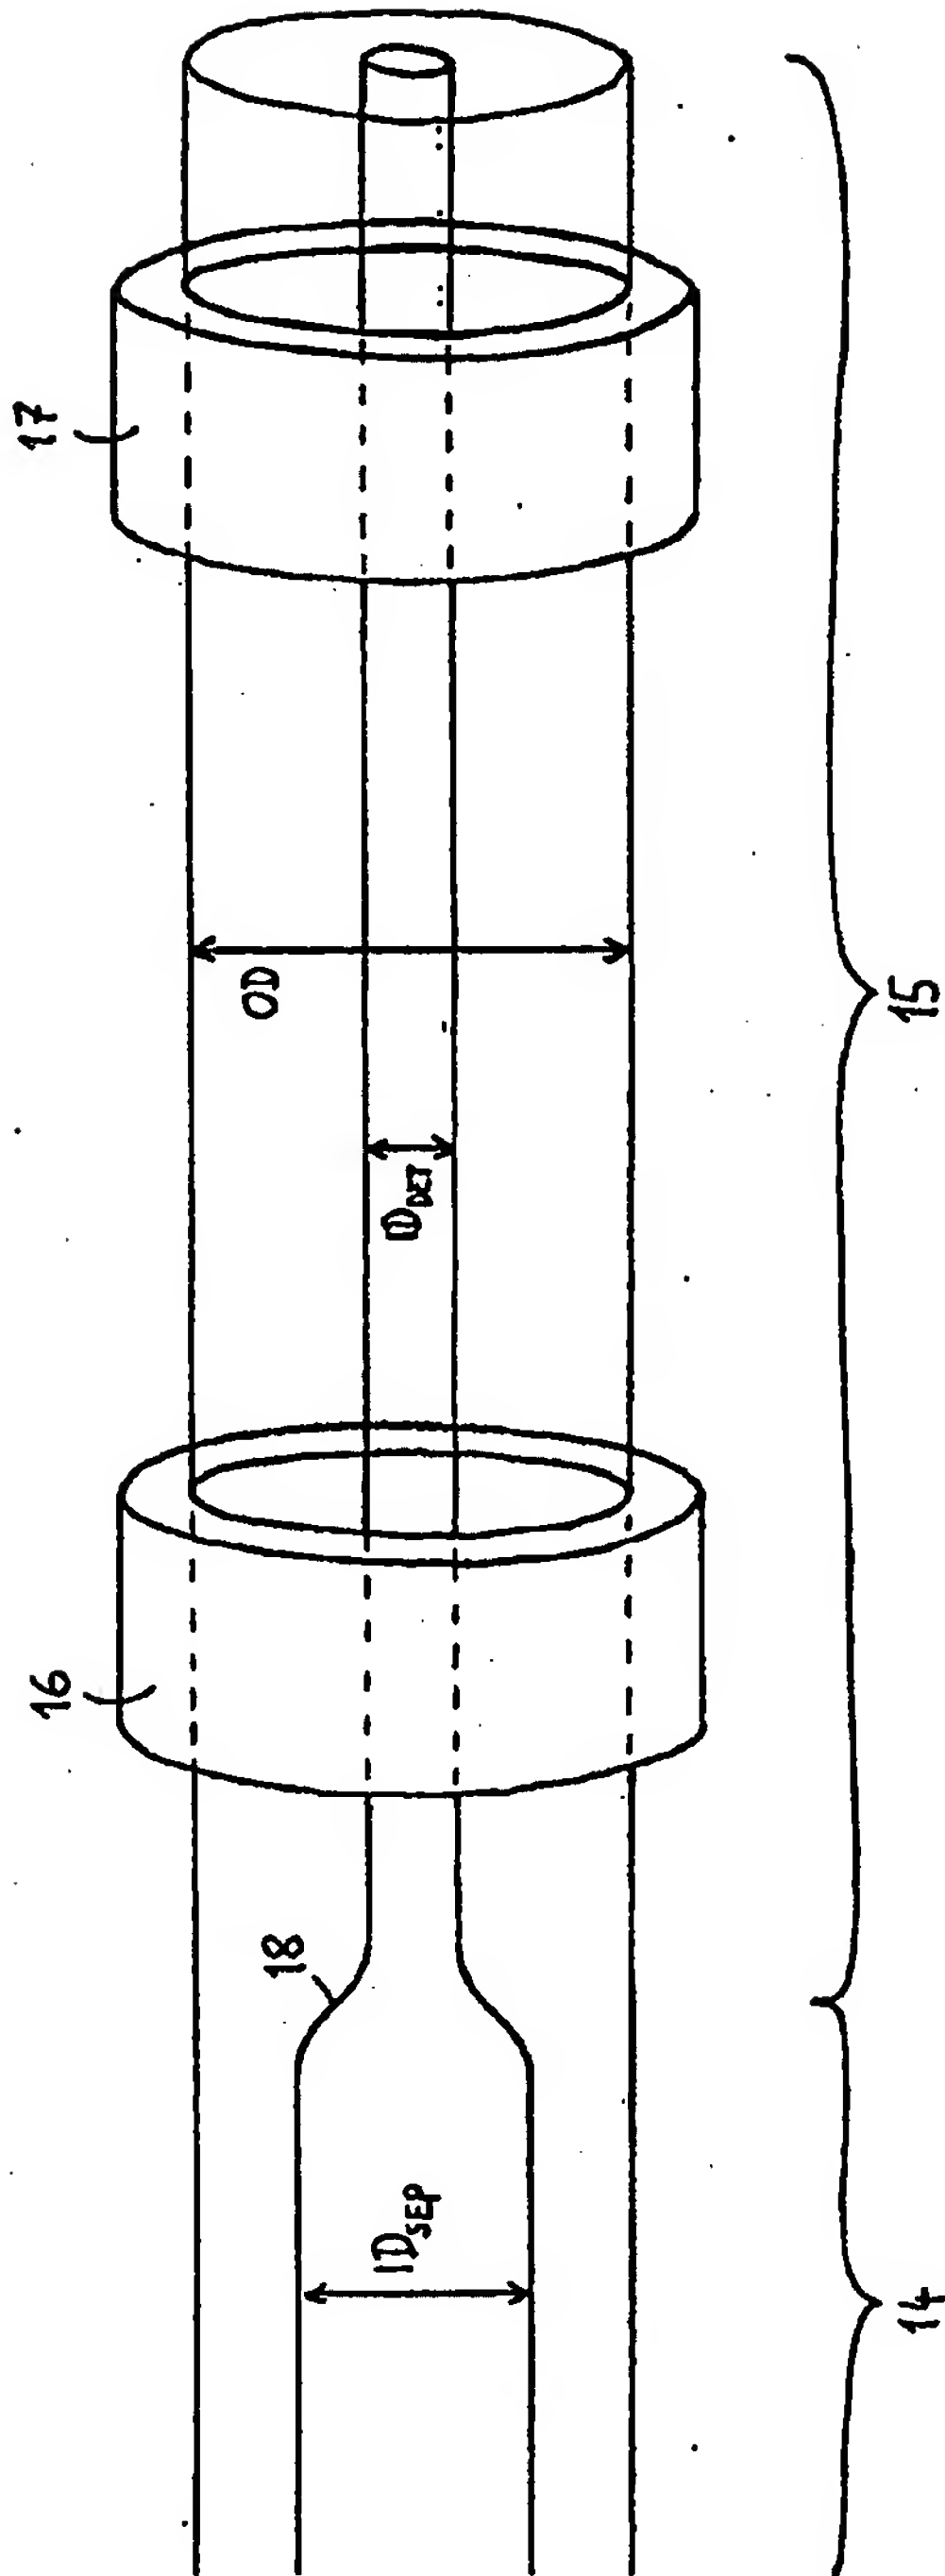


Fig. 2

BEST AVAILABLE COPY

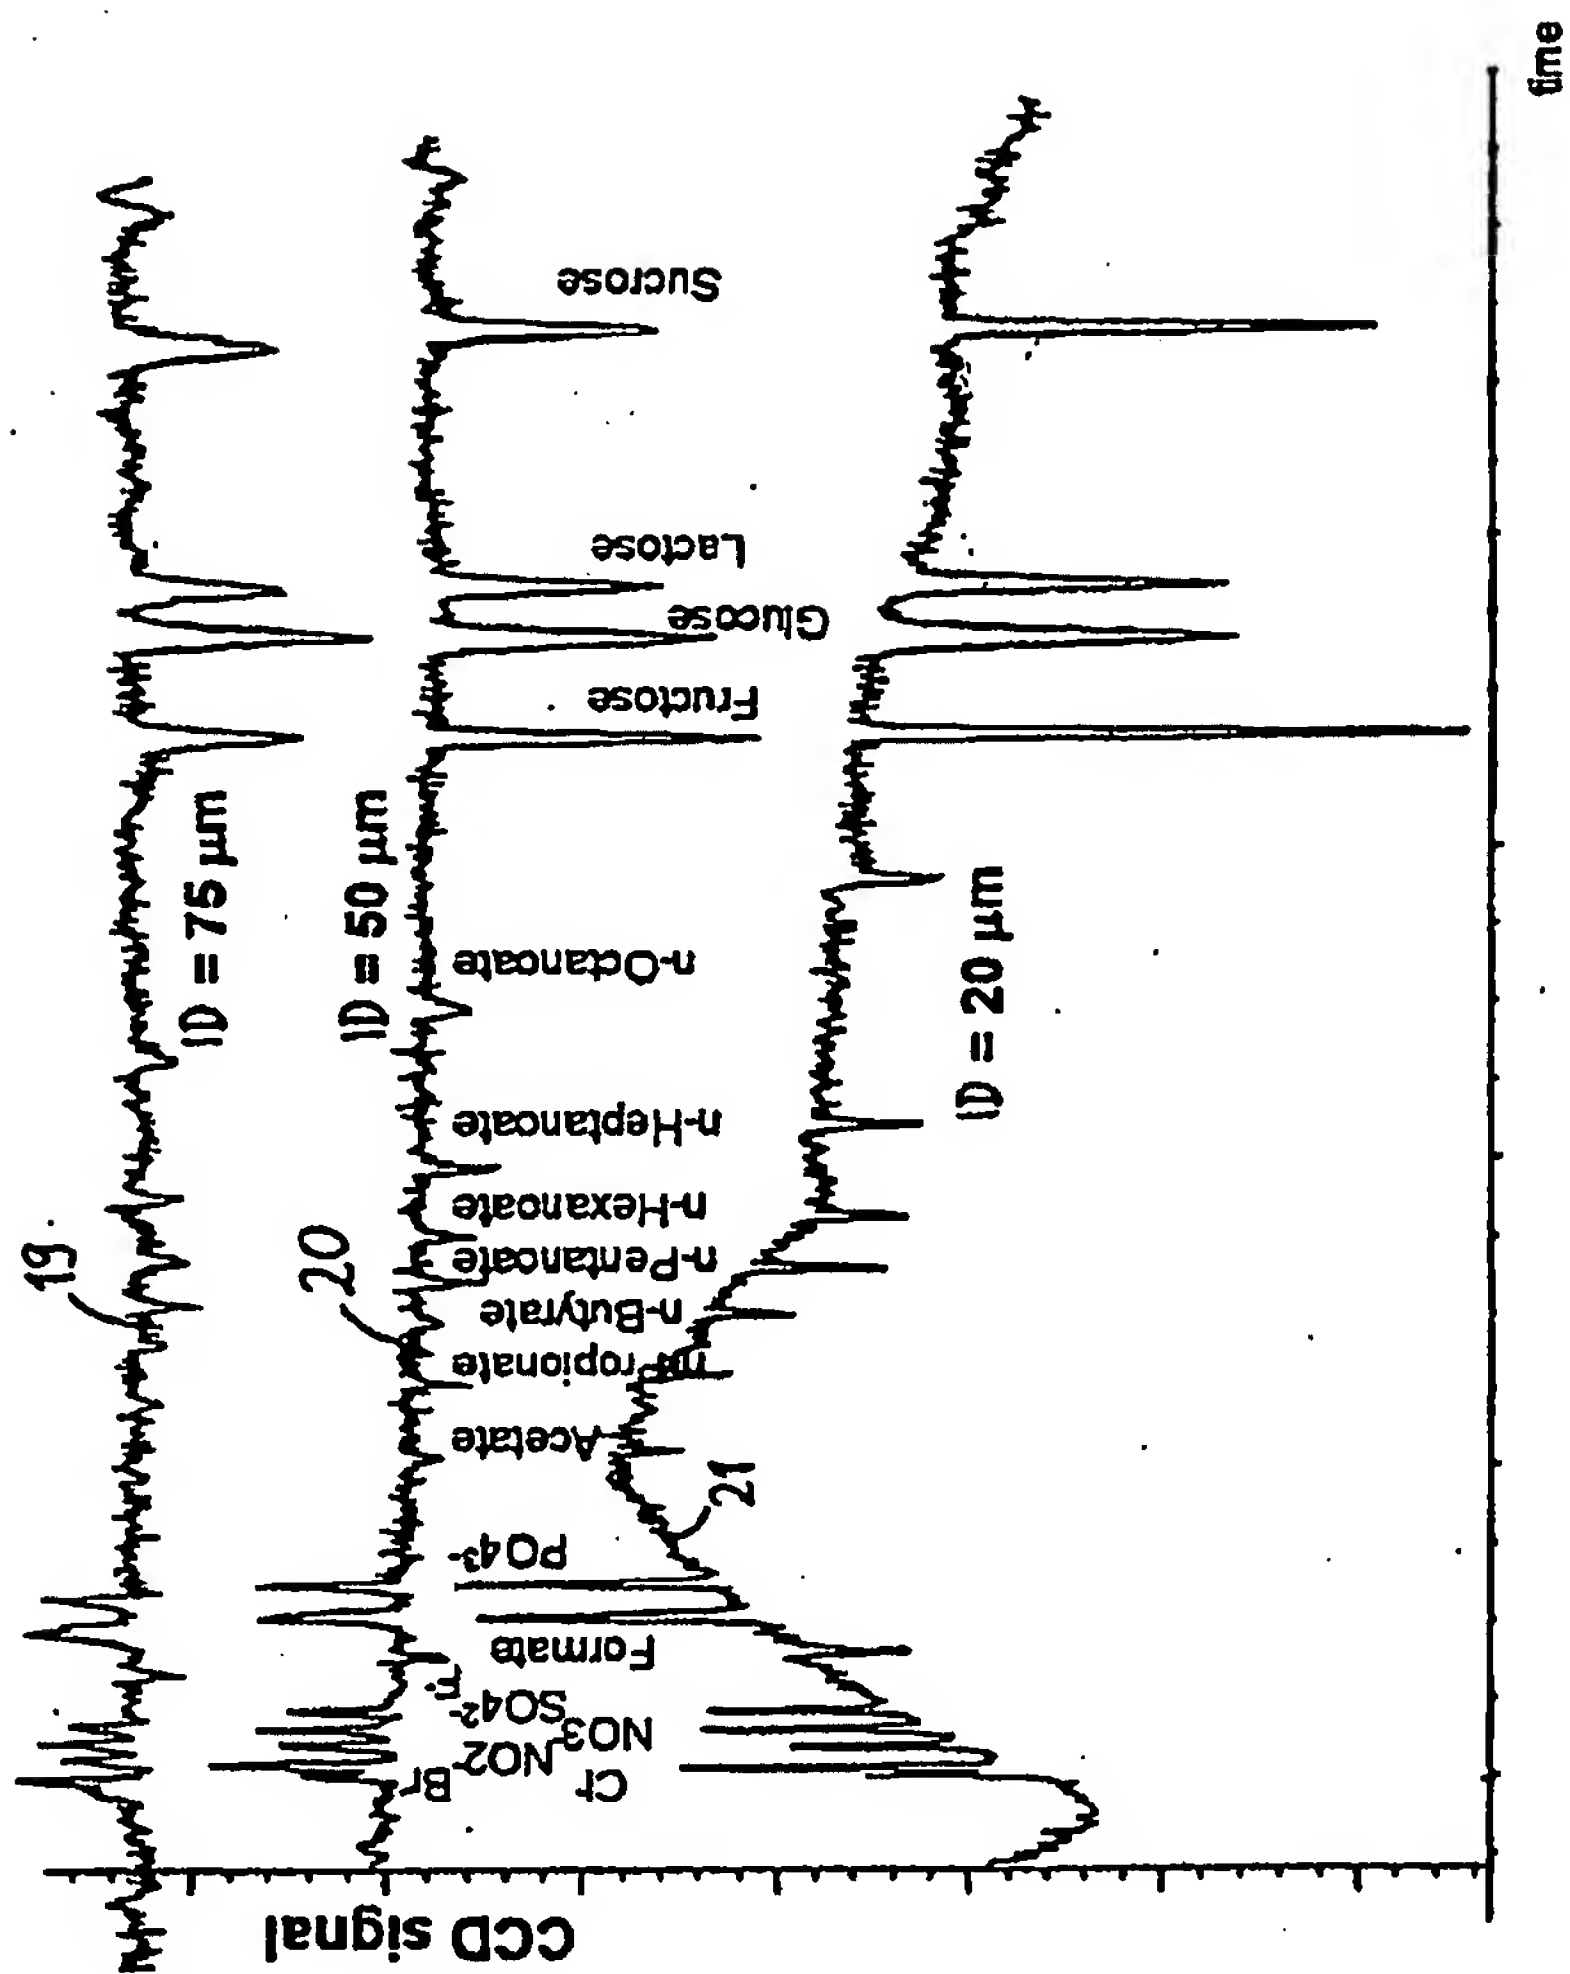


Fig. 3

BEST AVAILABLE COPY

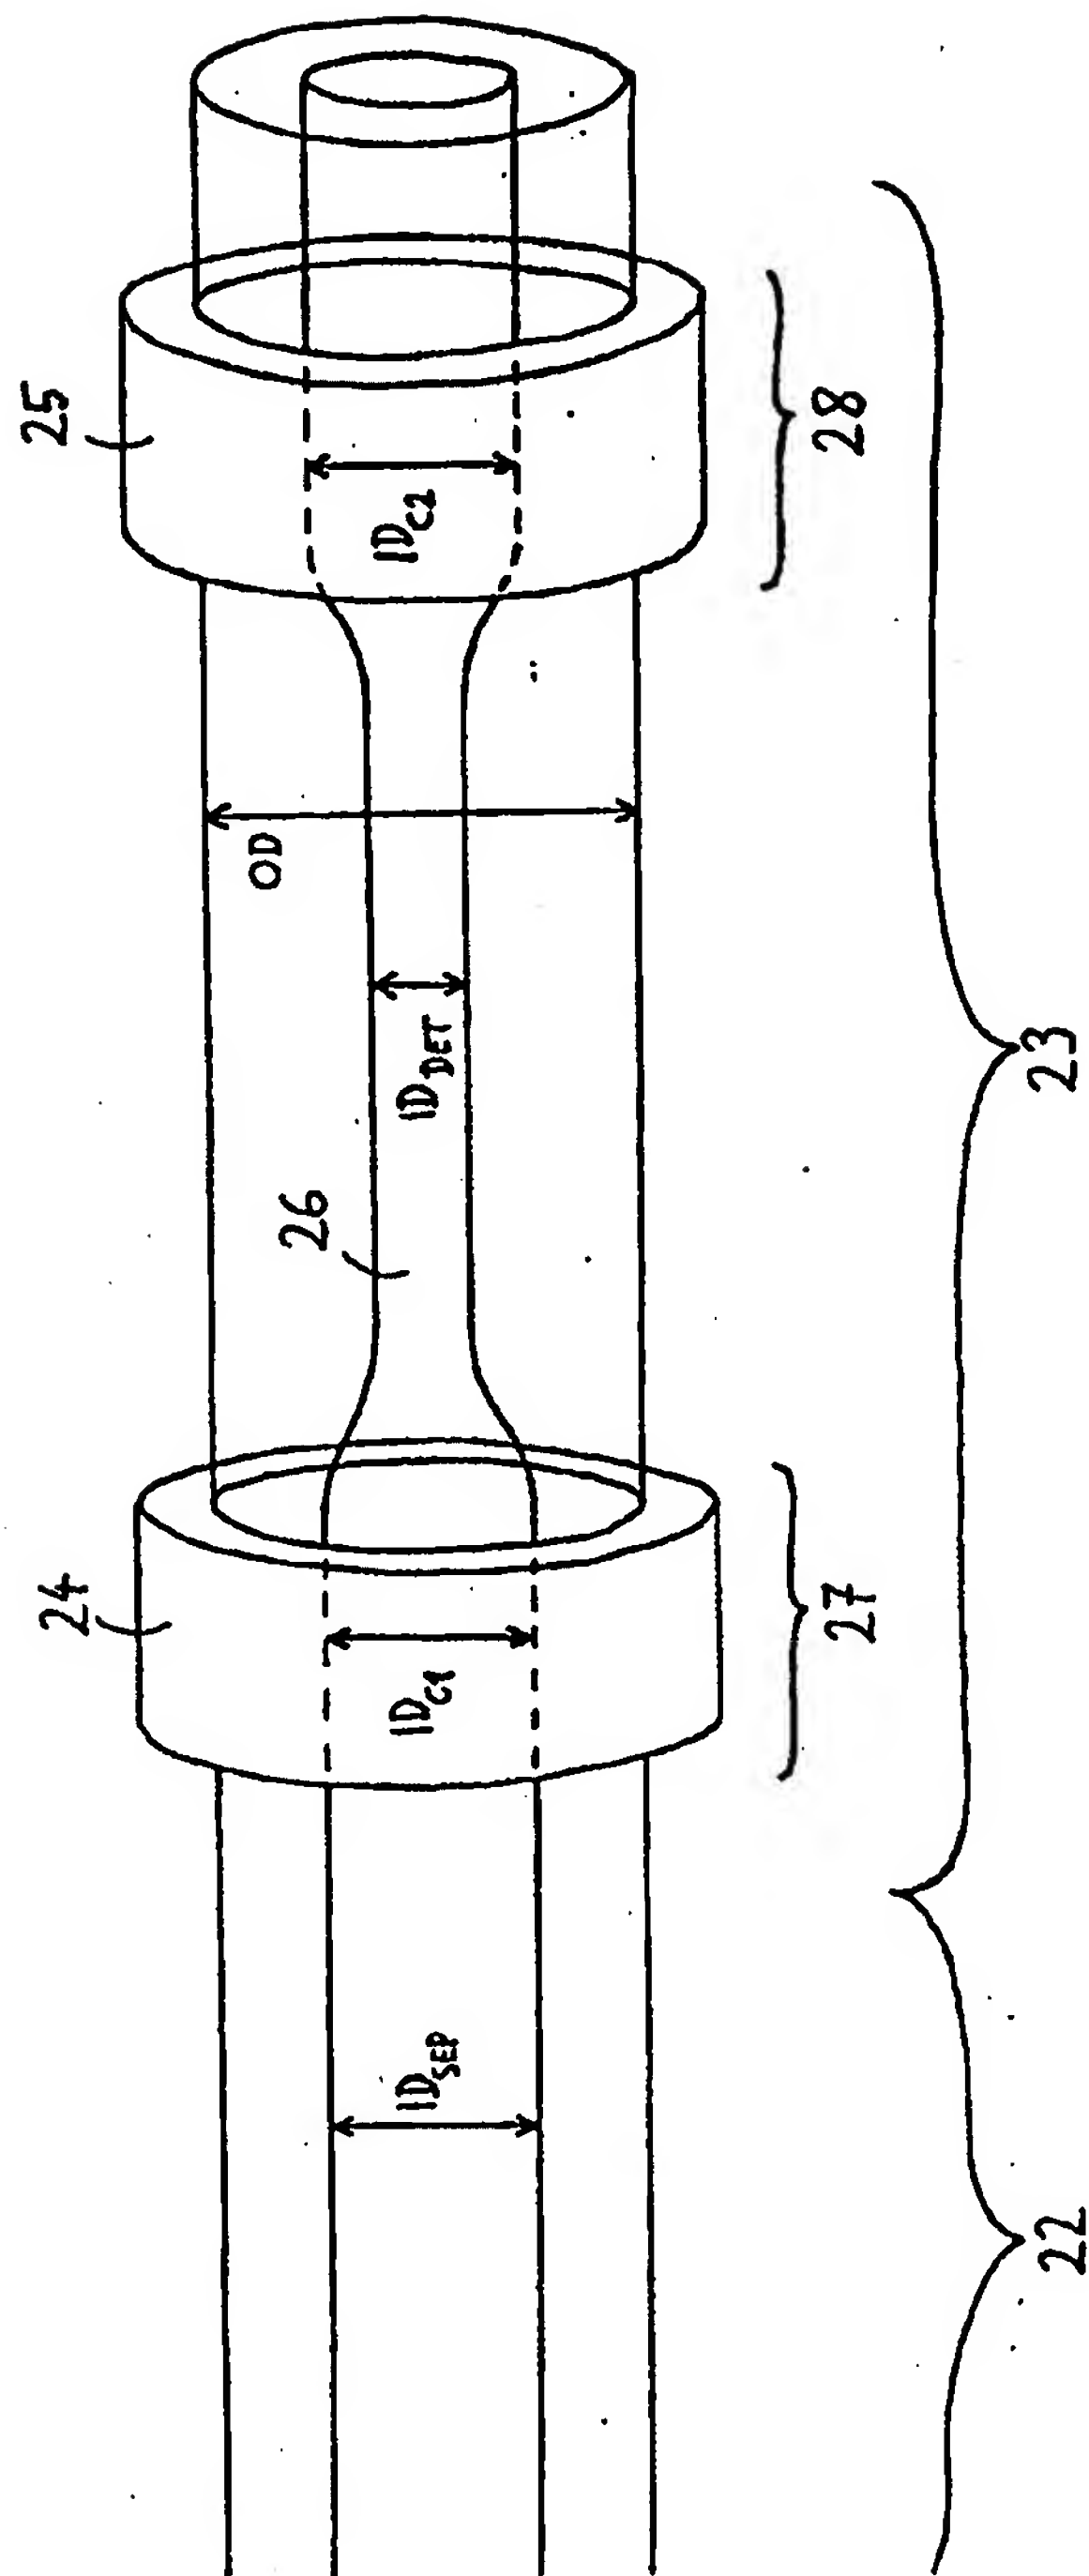


Fig. 4

BEST AVAILABLE COPY

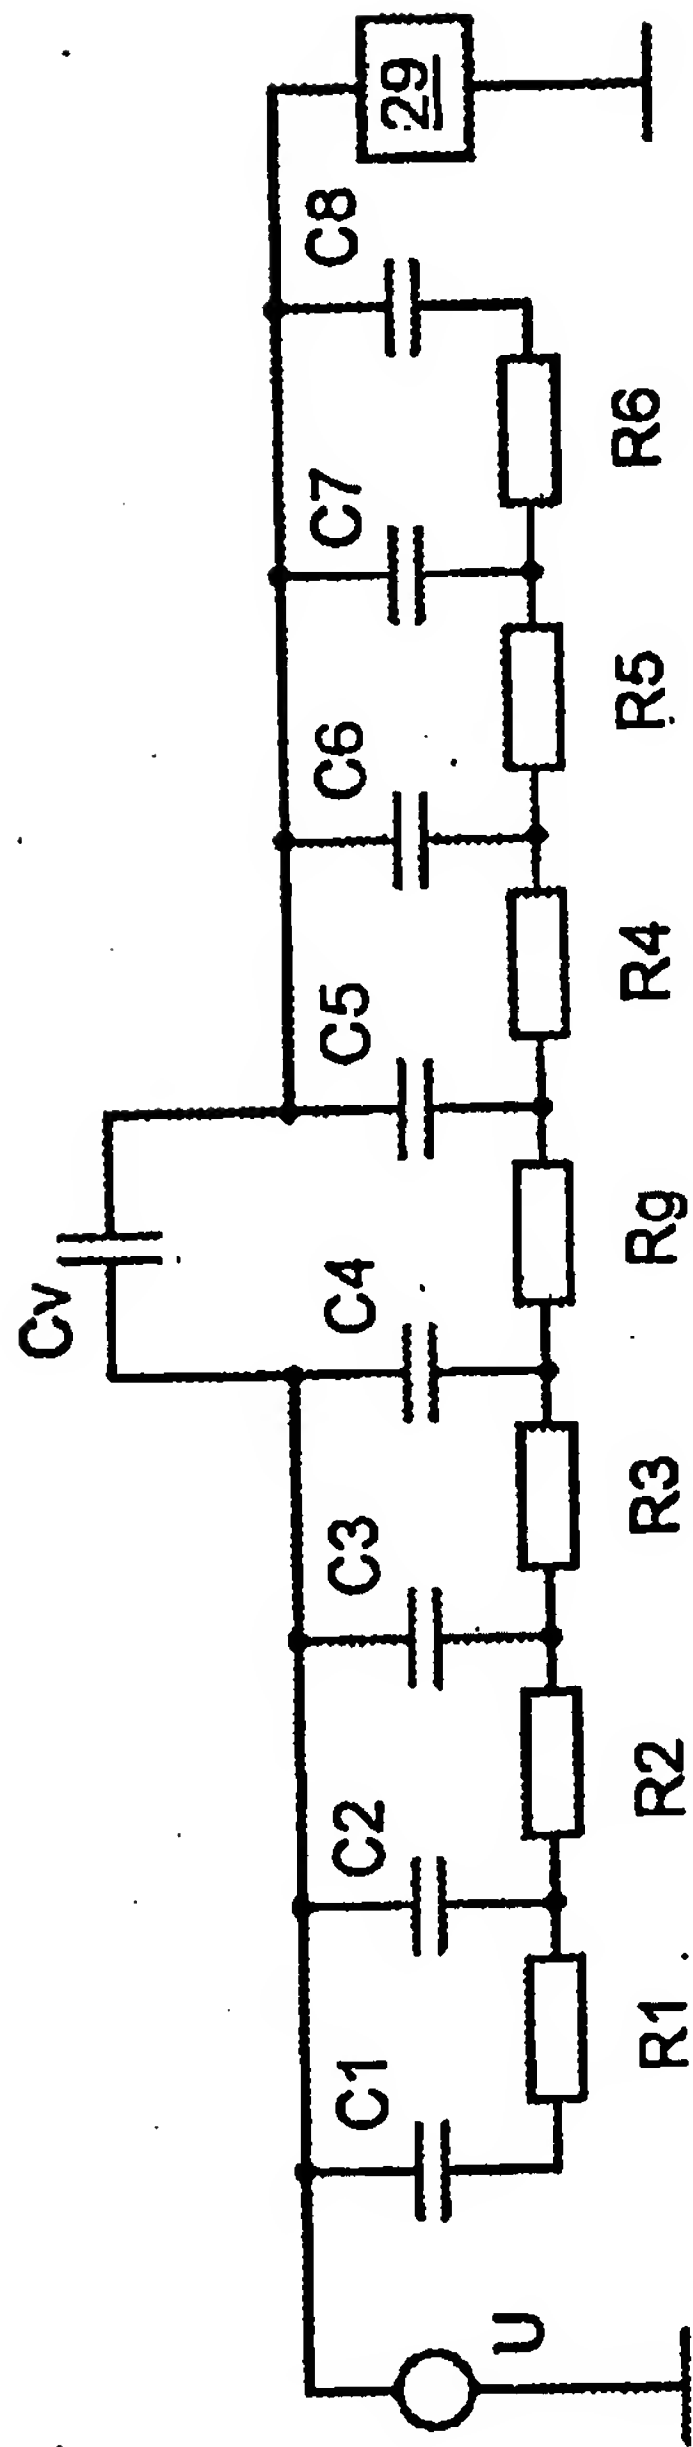


Fig. 5

BEST AVAILABLE COPY